SKIN+ACT

Galvanic Facial Skin Care Unit

PRODUCT MANUAL

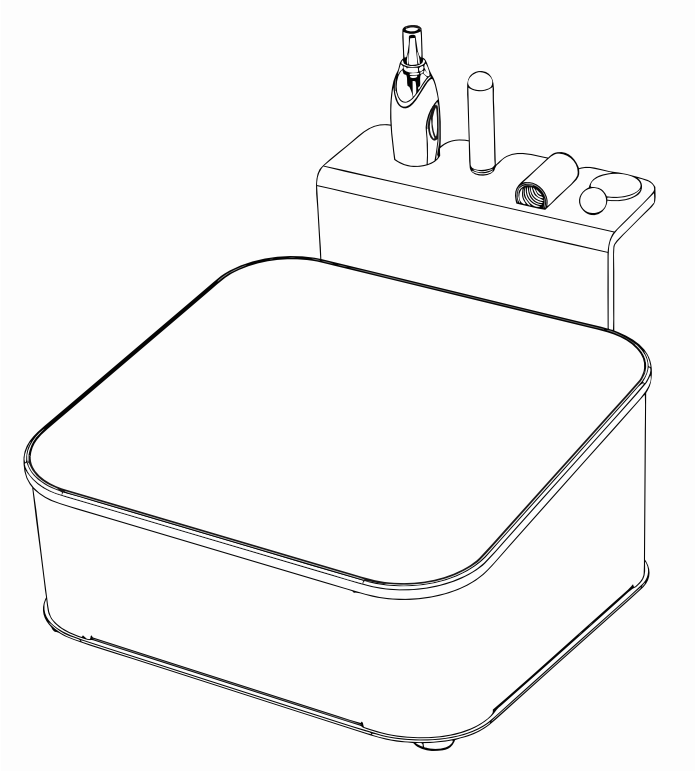

SKU25346

SKINACT.COM

NOTICE

No part of this document may be photocopied, reproduced, or translated into any other language with out prior written consent of Spa and Equipment/SkinAct.

The information in this document is subject to change without notice at any time and should not be construed as a commitment by Spa and Equipment/SkinAct

Spa and Equipment/SkinAct assumes no responsibility for an errors that may be in this document, nor does it make expressed or implied warranty with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

Spa and Equipment/SkinAct shall not be liable for incidental or consequential damages arising out of the furnishing, performance, or use of this document and the program material which it describes.

Thank You For Purchasing This Product!

Please read the entire instruction manual carefully before using the product. Take note of any warnings included in this manual.

Always keep this instruction manual handy and if you give the device to another person, hand over the manual as it is an essential part of the product.

Some components of the product may differ from the image that appears in catalogues, websites, brochures, ect..

In order to enhance the product, the manufacturer reserves the right to modify its features and/or components without prior notice.

Copyright © 2026 SkinAct, All Rights Reserved

TABLE OF CONTENTS

Disclaimer & Contraindications 4

Precautions & Important Notes 5

Included Items 7

Device Components 8

Device Components (Control Panel) 9

Assembly Instructions 10

Ion Introduction & Usage 11

Specifications 13

Warranty Information 14

DISCLAIMER

- This product has been designed to be used by esthetic professionals at spas and salons, it should not be used for other purposes.
- Please note that any misuse of the device entails the loss of the guarantee.
- Do not make any modification to the device without the authorization.
- We shall not be held liable for any material or personal damage due to the misuse of the product.
- Documents are made available without warranty of any kind. They may be updated, altered, expanded, or removed at any time. Skin Act does not warrant or guarantee any of the processes described herein or perform any independent analysis in connection with guidelines provided.
- Readers are expressly warned to consider and adopt all safety precautions indicated herein and to avoid all potential hazards. By following the instructions provided, the reader willingly assumes all risks in connection with such instructions.
- If the reader has questions about any of the guidelines provided by SkinAct we recommend they contact their nearest Esthetician Training Center to obtain more explicit instruction on Facial Machine Usage.

Contraindications

THIS DEVICE SHOULD NOT BE USED ON CLIENTS WITH:

- Pacemakers, metallic implants, or other electronic medical devices.
- Heart conditions or a history of heart disease.
- Pregnancy.
- Inflamed, irritated, or damaged skin.
- Severe acne rosacea or vascular conditions.
- Epilepsy or other seizure disorders.
- Clients undergoing medical treatments or with underlying health conditions must obtain prior clearance from a physician.

Precautions

- **Inspect the Device:** Check for any visible damage to the device or its power cable before and after each use.
- **Unplug When Not in Use:** Always disconnect the device from the power source before cleaning, storing, or performing maintenance.
- **Avoid Humidity:** Do not operate the device in bathrooms or other excessively humid environments.
- **Position Cables Safely:** Ensure the power cable is positioned to prevent tripping hazards and is plugged into a grounded socket.
- **Keep Away from Children:** The device and its accessories should be stored securely out of reach.
- **Report Issues Promptly:** If you notice abnormal functioning, contact your distributor or an authorized technician immediately.

Important Notes

- The iontophoresis treatment should be performed after cleansing and exfoliation, and before massage. Ensure the skin is clean and dry to prevent residue from being absorbed.
- Wrap the probe with cotton before use. Gradually increase the current from low to high, allowing the client to adapt while maintaining a mild tingling sensation.
- During treatment, do not touch the metal parts of the probe with your hands.
- This treatment is suitable for dry (dehydrated), mature, and oily skin. Select skincare products appropriate for the skin type. Avoid heavy oil-based products, as they may reduce penetration effectiveness.
- After treatment, clean the roller thoroughly and store it in a dry place to protect the electroplated surface.
- When the polarity is set to positive (+), the sensation is typically stronger than when set to negative (–). Adjust according to client comfort.
- Clients must remove all metal jewelry before treatment. This treatment is not suitable for individuals with metal implants (including gold teeth).

- Do not use on clients with sensitive skin, injuries, inflammation, telangiectasia, or during pregnancy.
- The acidity or alkalinity of the nutrient solution must match the polarity:
  - Positive (+): Use acidic solutions (Vitamin C, Collagen, Salicylic Acid)
  - Negative (−): Use alkaline solutions (Scaling Gels, Sodium Bicarbonate)
  - If unclear, test with pH strips before use
- Do not allow metal parts of the roller or probes to touch each other during operation. If contact occurs, the device's protection system will activate. Separate immediately to resume normal function.
- Keep the probe clean at all times. Clean and disinfect the probe after each use.
- Note: If using alcohol for disinfection, wipe only the metal parts of the probe. Do not apply alcohol to other parts, as this may cause damage.

Included Items

Qty	Part Name	Image
1	Host Machine	
1	Accessory Rack	
1	Galvanic Handle	
1	Power Adapter	

Device Components

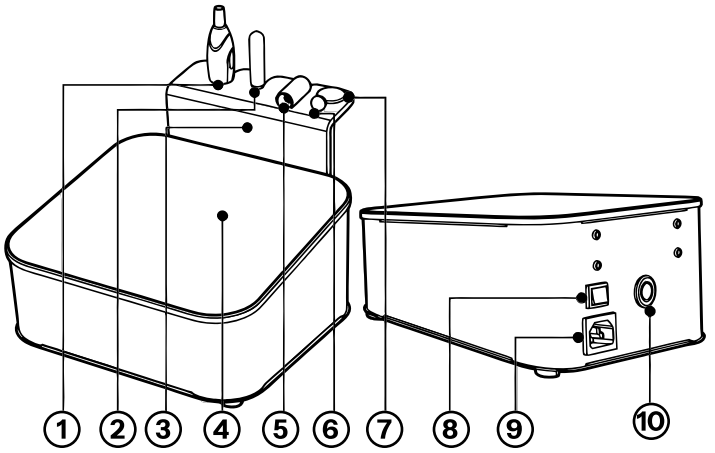

1. Galvanic Handle
2. Galvanic Grip
3. Attachment Rack
4. Control Panel
5. Roller Probe (Face)
6. Round Probe (Eye)
7. Sphere Probe (Face)
8. Power Switch
9. Electric Socket
10. Galvanic Port

Galvanic Handle

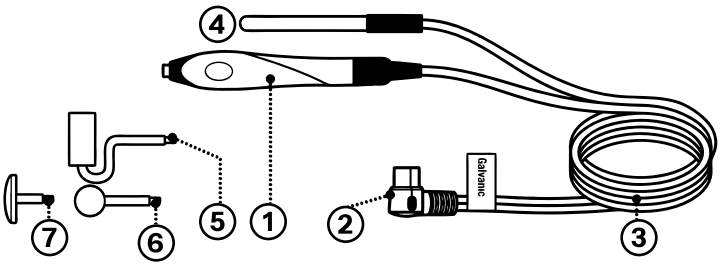

1. Conduction Probe
2. Galvanic Handle Plug
3. Galvanic Handle Cable
4. Galvanic Grip
5. Roller Probe (Face)
6. Round Probe (Eye)
7. Sphere Probe (Face)

Device Components (Control Panel)

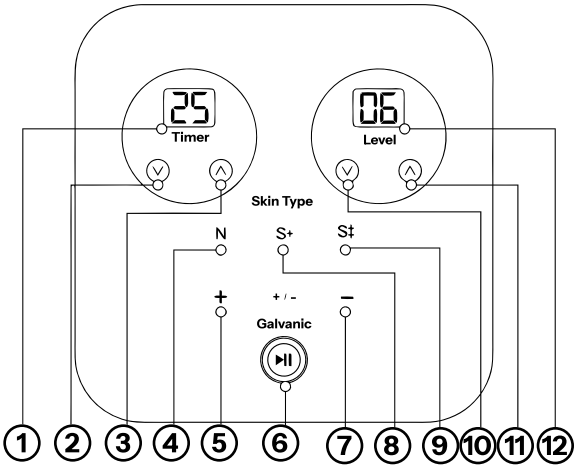

1. Timer Display
2. Timer Decrease
3. Timer Increase
4. Normal Mode
5. Cation Introduction
6. Start/Pause Button
7. Anion Introduction
8. Sensitive Mode
9. Extremely Sensitive Mode
10. Energy Level Decrease
11. Energy Level Increase
12. Energy Level Display

Assembly Instructions

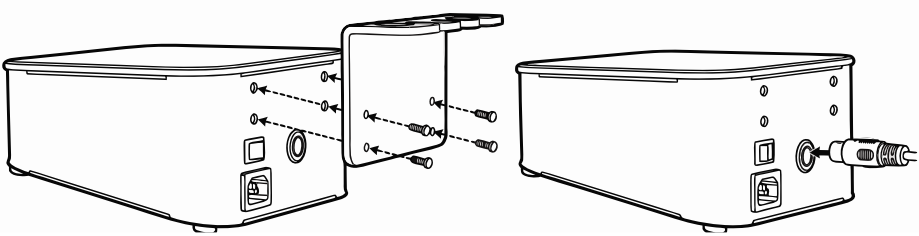

1. Secure the attachment rack to the back of the main unit using screws, following the direction of the arrows.
2. Place each attachment onto the rack.
3. Insert the handle into the corresponding port on the front of the main unit. Preparation is now complete.
4. Connect the power cord to the main unit.
5. Turn on the main power switch on the back of the device. The power light on the front will turn on, and the time display will show “15”. The energy display window will display “1”.
6. Select Polarity (Manual Control): Before starting treatment, manually select the required ion polarity based on your product's pH:
   - Press the Cation (+) for positive ion introduction.
   - Press the Anion (-) for negative ion introduction or deep cleansing.
7. Use the Level Increase/Decrease buttons to adjust the energy output. The adjustable range is Level 1 to Level 9.
8. Once the probe is in contact with the client, press the Start/Pause button to begin flow of current.

Ion Introduction Polarity Selection

- (+): Cation (positive ion) Introduction
- (-): Anion (negative ion) Introduction

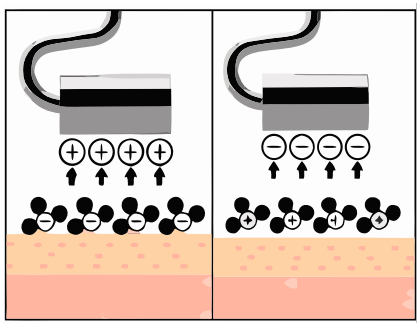

Usage (Iontophoresis Function)

A. Monopolar Infusion Method

1. Apply half of the nutrient solution directly to the skin. Soak the remaining solution into a cotton pad and wrap it around the probe.
2. Set the Level to minimum. Have the client hold the metal electrode rod while the operator holds the probe and places it on the treatment area.
3. Press the Start/Pause button to activate the device.
4. Select the required ion polarity (+ or −) based on the product used.
5. Gradually increase the Level until a mild tingling sensation is felt.
6. Move the probe slowly in a zigzag or circular motion, maintaining constant contact with the skin. (Figure 1)
    - Typical treatment time: 3–5 minutes

7. After completion:
   - Press Start/Pause to stop output
   - Turn off the Power
   - Remove the probe
   - Have the client release the electrode rod

Figure 1



B. Impurity Export (Deep Cleansing)

1. Set the working probe to negative (−) polarity. The client holds the positive (+) electrode rod..
2. Soak a cotton pad with saline or impurity-removal solution and wrap it around the probe, or apply gauze/mask to the treatment area.
3. Turn on the device and select anion (−) mode.
4. Start at a low energy level and increase gradually.
5. Move the probe slowly across the treatment area, keeping full contact with the skin.
6. After treatment, reduce energy to minimum, stop the device, and remove the probe.

C. Alternating Output Mode

1. Follow the same procedure as Method A (Monopolar Infusion).
2. In this mode, the device automatically alternates between positive and negative currents.
3. The polarity switches approximately every 0.5 seconds, providing continuous electrical stimulation to the skin. The rapid switching between positive and negative charges creates a "micro-massage" effect at the cellular level, which can help wake up sluggish or tired skin.

Specifications

Product Name:	Galvanic Facial Skincare Unit
Voltage:	AC100-120V/220-240V
Frequency:	50/60Hz
Power Consumption:	20W
Dimensions(L*W*H):	12x10x9 in
Net Weight:	3.7 lbs

Warranty Information

The manufacturer (the “warrantor”) warrants to the original purchaser that this equipment will be free from defects under normal and proper operation for a period of one (1) year from the date of purchase. This warranty covers all parts and labor for that one (1) year period. This warranty shall not apply to any equipment that has been subjected to abuse, misuse and alteration of any type or to any defect or damage caused by repair, replacement, substitution, or use with parts other than parts approved by the manufacturer. The manufacturer shall not be liable for the loss of use of this equipment, loss of time or business, inconvenience or any other indirect, consequential, special or incidental damages due to defects covered by this warranty or any implied warranty. To implement this warranty, contact the dealer from whom you purchased the equipment. If necessary, you will be asked to return all, or the appropriate part, of the equipment. If warranted, the repairs will be performed at no charge and the equipment returned to you. Unit owner must prepay all shipping costs when returning items for warranty service. This limited warranty is the only written or express warranty given by the manufacturer. This warranty gives you specific legal rights but you may also have other rights, which may vary from state to state or province to province.

SKIN+ACT

Phone: 1-800-418-0830
Email: info@skinact.com
Website: skinact.com